



U.S. Department
of Transportation

Pipeline and
Hazardous Materials
Safety Administration

East Building, PHH-23
1200 New Jersey Ave, SE
Washington, D.C. 20590

IAEA CERTIFICATE OF COMPETENT AUTHORITY
SPECIAL FORM RADIOACTIVE MATERIALS

CERTIFICATE USA/0723/S-96, REVISION 4

This certifies that the sources described have been demonstrated to meet the regulatory requirements for special form radioactive material as prescribed in the regulations of the International Atomic Energy Agency¹ and the United States of America² for the transport of radioactive material.

1. Source Identification - Varian Medical Systems Models 212 and 232.
2. Source Description - The Model 212 is a cylindrical single encapsulation made of stainless steel and either tungsten inert gas, laser, or plasma seal welded. Approximate outer dimensions of the encapsulation are 1.1 mm (0.04 in.) in diameter and either 3.36 mm (0.13 in.) or 4.96 mm (0.2 in.) in length. Minimum wall thickness is 0.17 mm (0.007 in.). A stainless steel connector and cable is welded to one end of the encapsulation. The overall length of the encapsulation, connector, and cable is 2,100 mm (82.7 in.). Construction shall be in accordance with either attached Varian Medical Systems Drawing Nos. GM212.13-020-SFC, Rev. D00 or GM212.13-010-SFC, Rev. D00. The Model 232 is a cylindrical single encapsulation made of stainless steel and either tungsten inert gas, laser, or plasma seal welded. Approximate outer dimensions of the encapsulation are 0.9 mm (0.04 in.) in diameter and either 2.97 mm (0.12 in.) or 4.52 mm (0.18 in.) in length. Minimum wall thickness is 0.08 mm (0.003 in.). A stainless steel connector and cable is welded to one end of the encapsulation. The overall length of the encapsulation, connector, and cable is 2,100 mm (82.7 in.). Construction shall be in accordance with either attached Varian Medical Systems Drawing Nos. GM232.03-000-SFC, Rev. E00 or GM232.02-000-SFC, Rev. D00.

¹ "Regulations for the Safe Transport of Radioactive Material, 2012 Edition, No. SSR-6" published by the International Atomic Energy Agency (IAEA), Vienna, Austria.

² Title 49, Code of Federal Regulations, Parts 100-199, United States of America.

CERTIFICATE USA/0723/S-96, REVISION 4

3. Radioactive Contents - No more than 51.8 GBq (1.4 Ci) of Iridium-192 for the short version of either Model or 555.0 GBq (15.0 Ci) of Iridium-192 for the long version of either Model. The Ir-192 is in the form of a solid metal.
4. Management System Activities - Records of Management System activities required by Paragraph 306 of the IAEA regulations shall be maintained and made available to the authorized officials for at least three years after the last shipment authorized by this certificate. Consignors in the United States exporting shipments under this certificate shall satisfy the requirements of Subpart H of 10 CFR 71.
5. Expiration Date - This certificate expires on February 28, 2026. Previous editions which have not reached their expiration date may continue to be used.

This certificate is issued in accordance with paragraph(s) 804 of the IAEA Regulations and Section 173.476 of Title 49 of the Code of Federal Regulations, in response to the January 19, 2021 petition by Varian Medical Systems, Palo Alto, CA, and in consideration of other information on file in this Office.



Certified By:




William Schoonover
Associate Administrator for Hazardous
Materials Safety

February 11, 2021
(DATE)



Revision 4 - Issued to extend the expiration date.

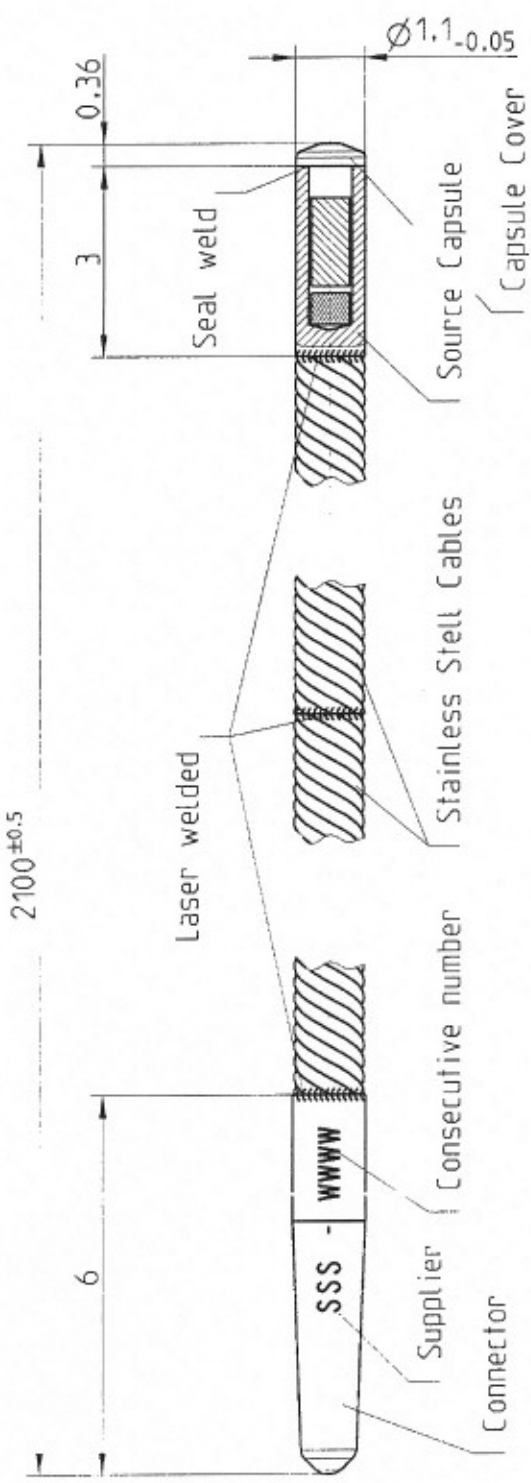


Engraving style until rev. C00:
(for reference only)



| | |
|--|--------------------------------|
| VARIAN medical systems | |
| Varian Medical Systems Inc., 3100 Hansen Way, Palo Alto, CA 94304, USA | |
| Name: | GammaMed 12i(t) 212 PDR Source |
| Drawing No.: | GM212.13-020-SFC |
| Model: | GM212-13-0200-ASM |
| Dwg: | GM212-13-0200-SFC.DRW |
| Rev: | D00 |
| Date: | 10/Jan/2007 |



Engraving style until rev. C00:
(For reference only)



Type designation






"001" to "999"
consecutive number



Connector with ID

Varian Medical Systems Inc.
3100 Hansen Way, Palo Alto,
CA 94304, USA

| | |
|--------------|--------------------------------|
| Name: | GammaMed 12i(t) 212 HDR Source |
| Drawing No.: | GM212.13-010-SFC |
| Rev.: | D00 |
| Model: | GM212-13-0100-ASH |
| Dwg.: | GM212-13-0100-SFC.DRW |
| Date: | 10/Jan/2007 |



| | |
|--|------------------------------|
| VARIAN medical systems Varian Medical Systems Inc., 3100 Hansen Way, Palo Alto, CA 94304, USA | |
| Name: | Gammamed plus 232 PDR Source |
| Drawing No.: | GM232.03-000-SFC |
| Rev: | E00 |
| Model: | GM232-03-000E-ASM |
| Dwg: | GM232-03-000E-SFC-DRW |
| Date: | 11/Jan/2007 |



Engraving style until rev. C00:
(for reference only)



Type designation



"001" to "999"
consecutive number

Connector with ID

VARIAN
medical systems

Varian Medical Systems Inc.,
3100 Hansen Way, Palo Alto,
CA 94304, USA

| | |
|--------------|------------------------------|
| Name: | GammaMed plus 232 HDR Source |
| Drawing No.: | GM232.02-000-SFC |
| Rev.: | D00 |
| Model: | GM232-02-0000.ASM |
| Date: | 11/Jan/2007 |
| Dwg.: | GM232-02-000000-SFC.DRW |



U.S. Department of
Transportation

**Pipeline and
Hazardous Materials
Safety Administration**

East Building, PHH-23
1200 New Jersey Ave, SE
Washington, D.C. 20590

CERTIFICATE NUMBER: USA/0723/S-96

ORIGINAL REGISTRANT(S) :

Varian Medical Systems
M/S LV1
6883 Spencer Street
Las Vegas, NV, 89119
USA